


**ACQCROSS™ QX**  
INTEGRATED TRANSEPTAL  
DILATOR/NEEDLE

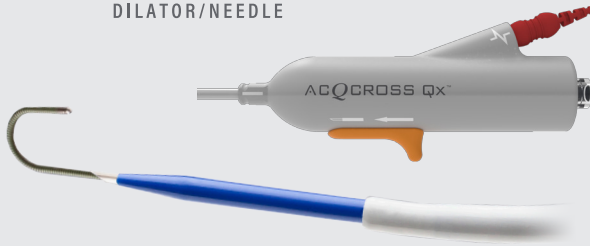


**WIRE + NEEDLE + DILATOR + INTRODUCER SET**

- Spring-tensioned safety needle; only deploys when actuated
- Integrated dilator/needle and introducer lock together as one unit for control and ease of use
- Reduce wire exchanges with retained guide-wire method
- Dual purpose needle; use mechanically or with RF energy
- Packaged as a convenient kit with Integrated dilator/needle, steerable or fixed curve introducer, guidewire, and ES and EGM cables


**ACQGUIDE™ FLEX**  
STEERABLE INTRODUCER

- Left-handed operation of introducer allows for simultaneous right-hand control of ablation catheters

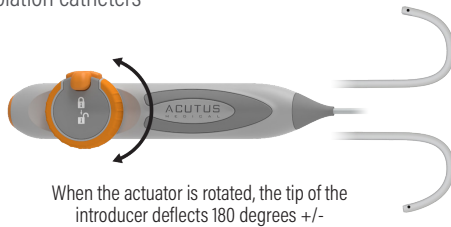


**ACQGUIDE™ MINI**  
FIXED-CURVE INTRODUCER


- Facilitate positioning with fixed distal curve and improved torquability

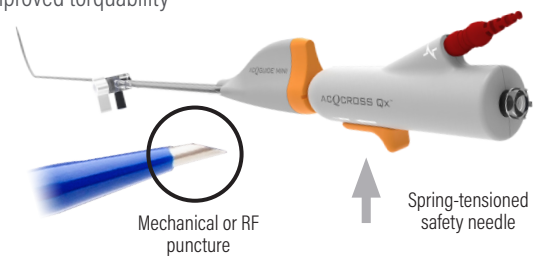


## AcQCROSS™ Transseptal Access Procedure




**STEP 1:** Insert AcQCROSS™ Qx into Superior Vena Cava (SVC).  
**Guidewire remains retained in dilator.**




**STEP 2:** Perform 'drag-down' to locate Fossa Ovalis. Guidewire is pulled back into lumen of dilator, **still retained.**




**STEP 3:** Confirm correct position and tent. **If repositioning is needed, re-advance guidewire back to SVC and repeat.**



**STEP 4:** Needle extended and advanced into the Left Atrium (LA). **Options: mechanical or RF puncture.**




**STEP 5:** With needle across, advance the guidewire into the LA.




**STEP 6:** With needle safely retracted, advance AcQCROSS Qx into the LA over the guidewire.

## AcQCross™ Qx Workflow

Half the steps of a traditional transseptal access workflow

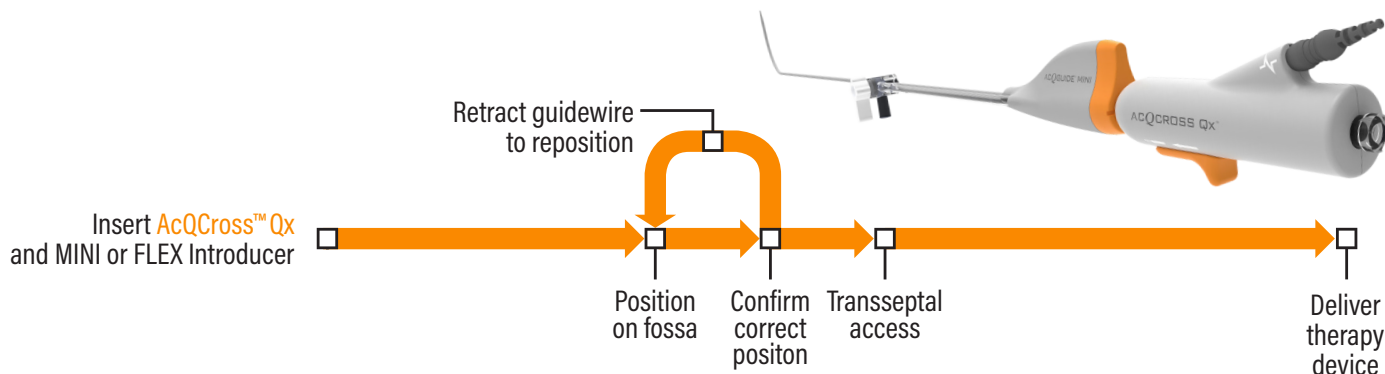

## Traditional transseptal access workflow

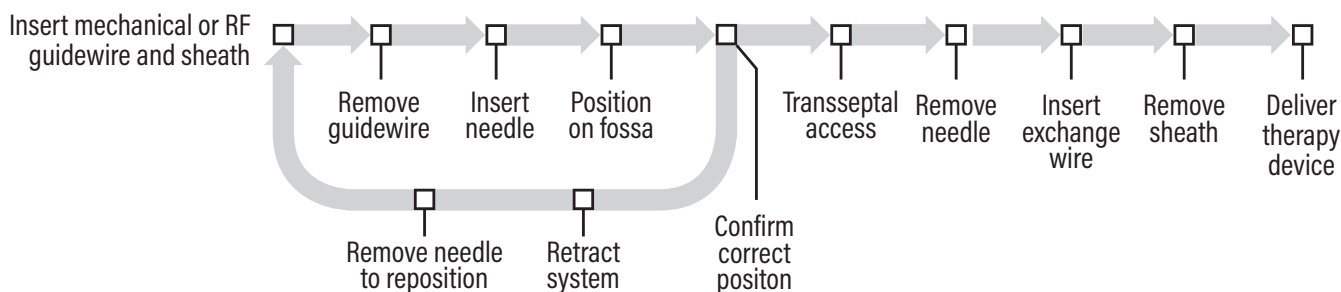

### ORDERING INFORMATION

#### Transseptal Access System for Mechanical or RF Energy Application

PRODUCT NAME	PRODUCT DESCRIPTION	PRODUCT CATEGORY	ITEM #
AcQGuide® FLEX 65 cm - MED Curl	65 cm, Med Curl, 8.5F ID, 12F OD	Steerable Introducer	122852
AcQGuide® FLEX with RF 65 cm - MED Curl	65 cm, Med Curl, 8.5F ID, 12F OD	Steerable Introducer	222852
AcQGuide® MINI 65 cm - L2	65 cm, 90 deg, 8.5F ID, 12F OD	Catheter Introducer	112852
AcQGuide® MINI with RF 65 cm - L2	65 cm, 90 deg, 8.5F ID, 12F OD	Catheter Introducer	212852
AcQGuide® MINI-S with RF 65 cm - L2	65 cm, 90 deg, 8.5F ID, 12F OD	Catheter Introducer	012852

**NOTE:** All Steerable and Fixed-Curve products packaged with appropriate length AcQCross™ Qx Transseptal Dilator/Needle (8.5F OD)

#### WIRE + NEEDLE + DILATOR + INTRODUCER SET

A simplified, optimized workflow for improved efficiency and safety.

Prior to using these devices, please review the Instructions for Use for a complete listing of indications, contraindications, warnings, precautions, potential adverse events, and directions for use. The AcQGuide® MINI with AcQCross™ Qx and AcQGuide® FLEX with AcQCross™ Qx devices are FDA cleared. [acutus.com/patents](http://acutus.com/patents)

Acutus Medical®, Acutus®, AcQMap®, AcQGuide® and AcQRef® are registered trademarks of Acutus Medical, Inc. AcQCross™ Qx, AcQGuide® FLEX, AcQGuide® MINI are trademarks of Acutus Medical. This material is the property of Acutus Medical and its subsidiaries. Please do not copy, forward, or distribute this document. Copyright © 2020 Acutus Medical, Inc. All rights reserved.

**ACUTUS MEDICAL, INC.**  
2210 Faraday Ave, Suite 100  
Carlsbad, CA 92008 United States  
Phone: 888-202-8151  
[acutus.com](http://acutus.com)

**ACUTUS™**  
M E D I C A L